



# SERVICE BULLETIN

---

## KODAK X-OMAT Processor

---

Eastman Kodak Company/Customer & Technical Services/Health Sciences Markets Division/Rochester, New York 14650

SERVICE BULLETIN NO. 158

April 1993

### **Kodak PROCESSORS**

#### **Kodak AUXILIARY VENTILATION FAN KIT/110 V**

The *Kodak* AUXILIARY VENTILATION FAN KIT/110 V is available for use with all *Kodak* PROCESSORS. The Kit is designed to aid in meeting site specifications for ventilation. Improperly vented processors may exhibit film artifacts and corrosion of internal metal parts and accessories attached to processors. The Kit should be installed whenever ventilation is inadequate or marginal. **See Service Bulletin No. 101, October 1992, for correct dryer exhaust venting procedures.**

#### **NOTE**

The FAN must be connected to a building's exhaust that forces air to the outside of the building, so that no air is reused.



The Kit is stocked at Service Parts Management under Part No. 264503. Spare parts are also stocked at Service Parts Management. 1-800-431-7278

The Kit allows installation of the FAN and AIR GAP to either a wall or a pillar, or to the exhaust duct itself if the duct is strong enough to support the weight of the FAN. Adjustment of the AIR GAP allows the accurate control of air flow so that processor ventilation meets site specifications. The AIR GAP is designed so that it can be used with either 3-inch or 4-inch diameter exhaust ducts.

Installation Instructions for the *Kodak* AUXILIARY VENTILATION FAN KIT/110 V, publication number 981914, dated 2/93, provide installation, operation, and parts list information. The publication is included with the FAN KIT or can be ordered separately from Service Parts Management.

For more information, please contact:

Eastman Kodak Company  
Customer Service and Sales Support  
Health Sciences Division  
100 Carlson Road  
Rochester, New York 14653-9013  
(716) 724-1789

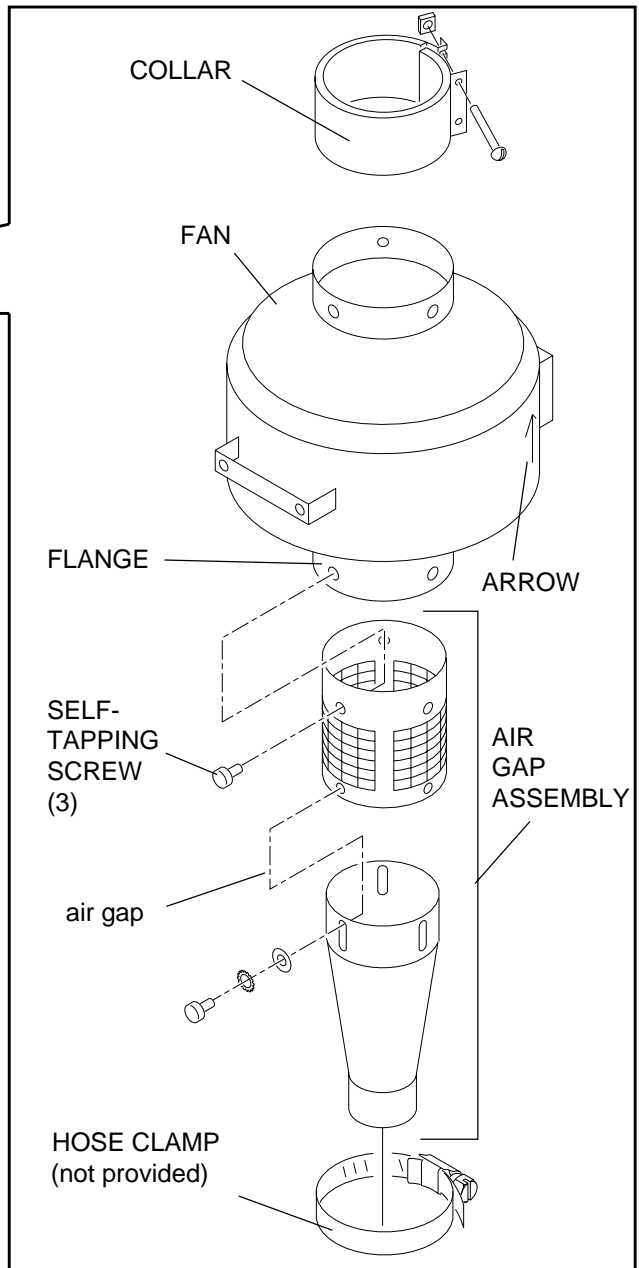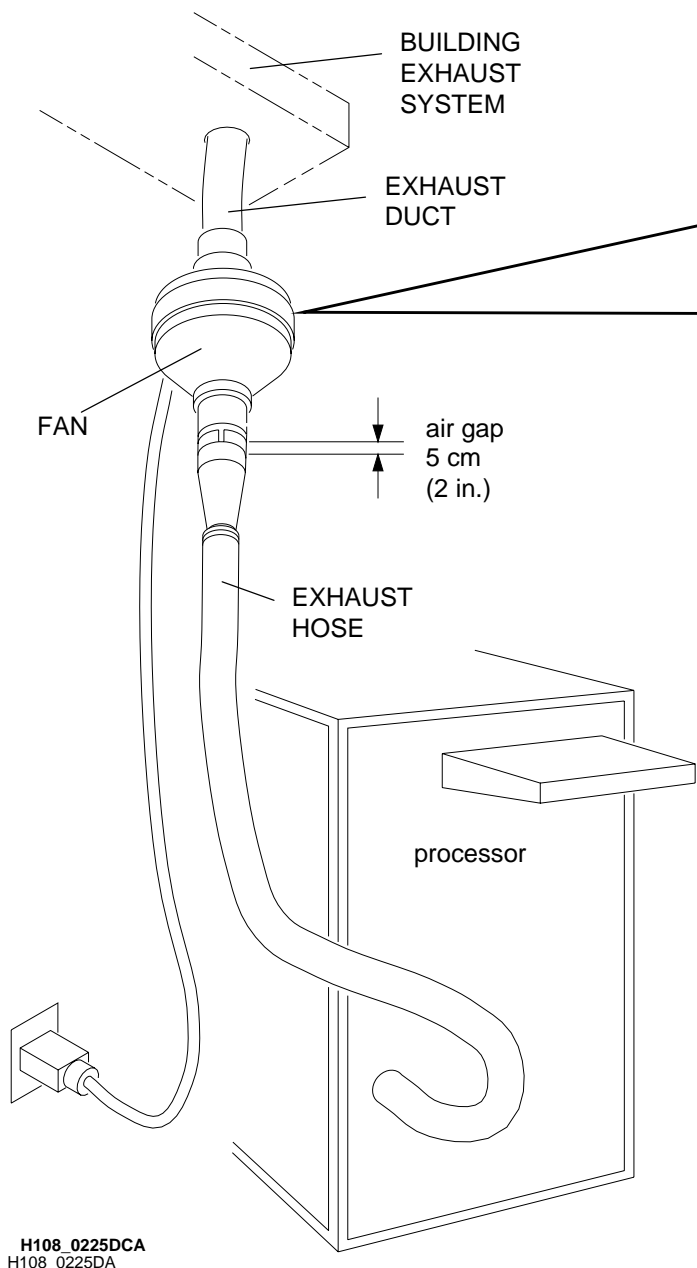

svcbul\_158.txt  
N-768

*Kodak* is a trademark.

